



MOBIDERM



SLEEVES (All Fields are Mandatory)

ORDER (by default) **QUOTATION** **RENEWAL**

Customer code

Case No. for renewal

1st treatment

Date: _____ Quantity: _____

CLINICIAN IDENTIFICATION

NAME: _____

EMAIL: _____

PHONE: _____

Patient's surname: _____

Patient's first name: _____

Gender: M F Child Patient's height: _____

I authorize my health care professional to collect my data and to communicate them to Thuasne company as part of the processing of my made to measure medical device in accordance with Law No 78-17 of 6 January 1978, and European Regulation No 2016/679/EU of 27 April 2016, I have rights including in particular the rights of access, rectification, portability and deletion of my data. I can exercise these rights by contacting the health care professional from whom I ordered my medical device.

PATIENT SIGNATURE

If possible, please enclose photos of the limb to be fitted. Please draw in the contours of the garment on the diagram and cross unnecessary measures.

RIGHT ARM **LEFT ARM**

Fill out one form for each side

FACING VIEW

Models

- Armsleeve (big blocks only)
- Armsleeve with mitten with thumb (big blocks on the arm and small blocks on the hand)
- Armsleeve with mitten without thumb (big blocks on the arm and small blocks on the hand)

Sleeve options

- Anti-slip with silicone dots 3 cm
- Velcro opening

Comments

.....


.....

.....

.....

.....

.....

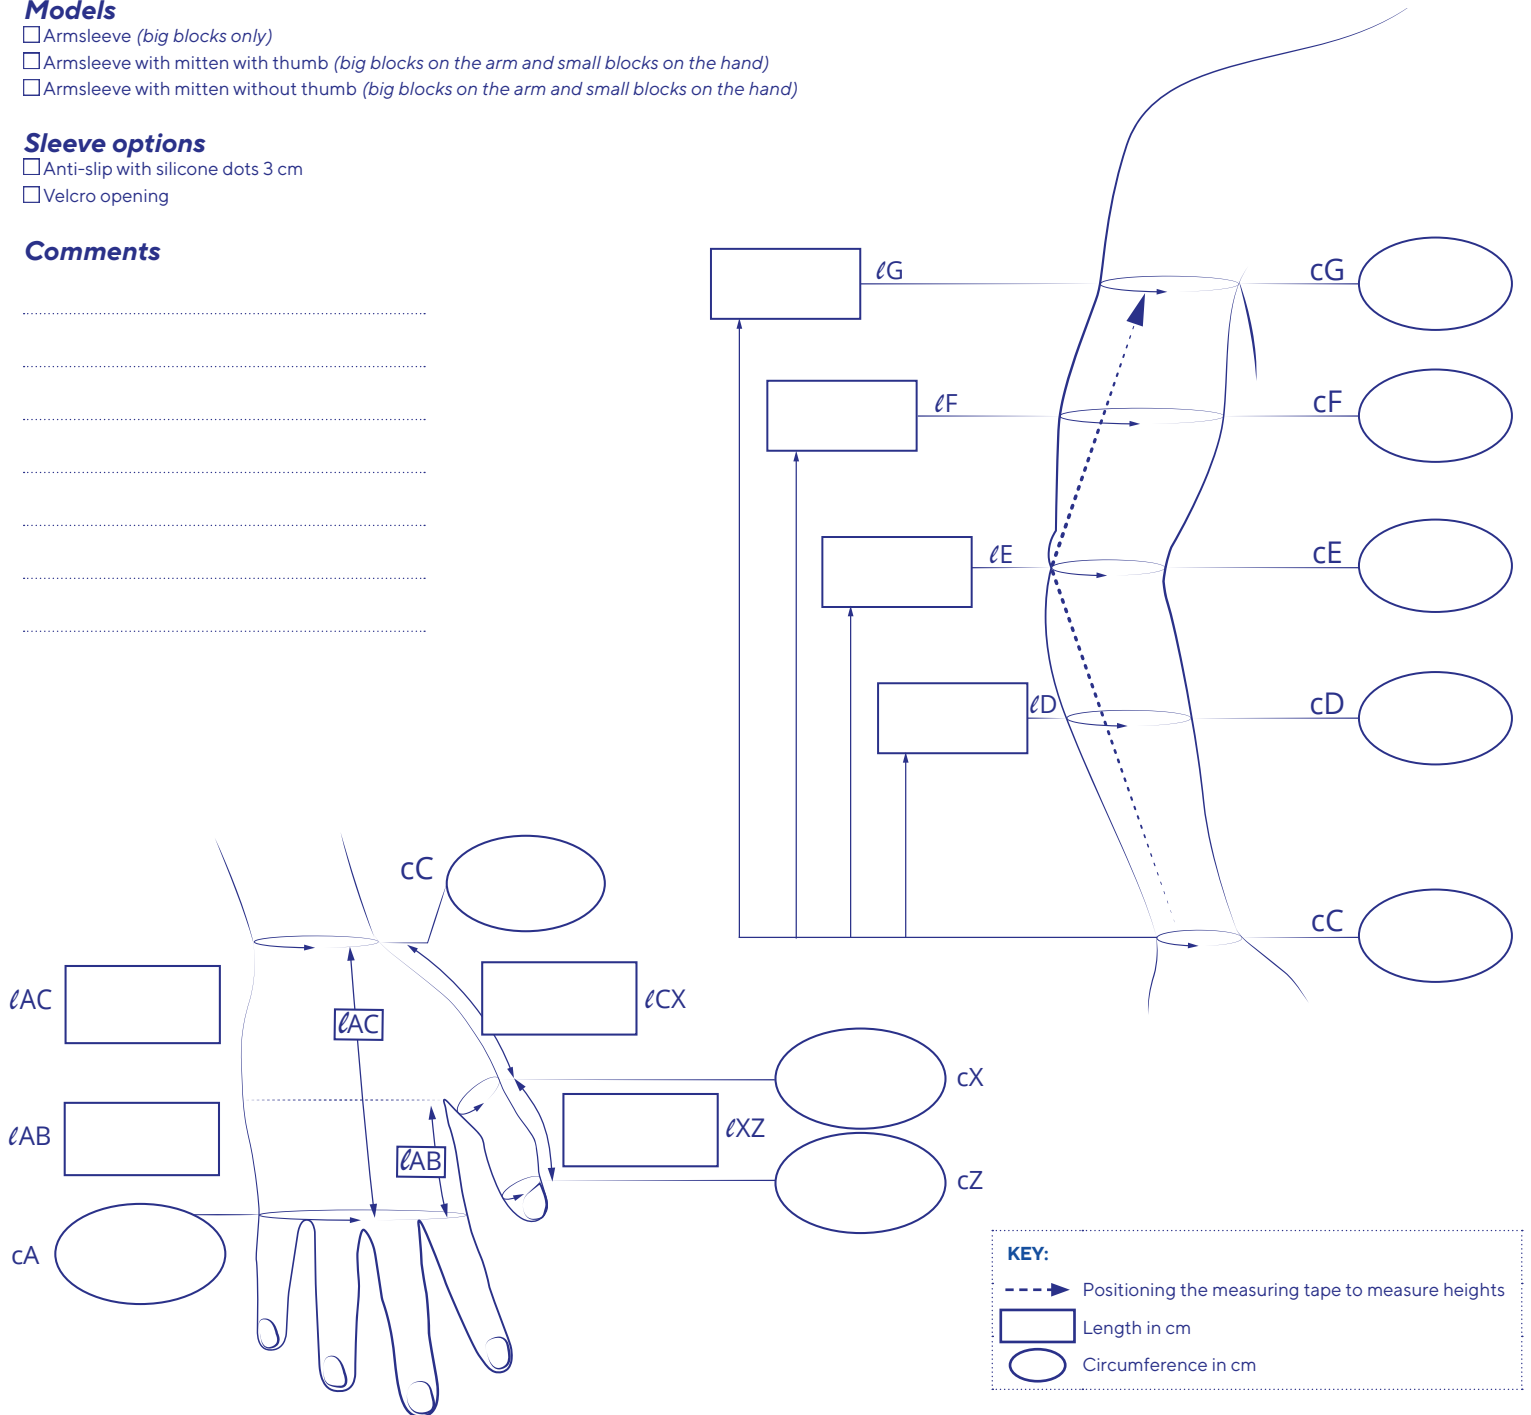

Please send completed form and any queries to: orders@thuasne.co.uk

MOBIDERM

SLEEVES


Anatomical Markers

- Ⓒ corresponds to the axilla (armpit)
- Ⓕ corresponds to the widest point of the biceps
- Ⓖ is located at the level of the olecranon
- Ⓓ equidistant between A and C or at the starting site of the edema
- Ⓒ to be measured at the narrowest point of the wrist external face in the middle of the radial ulnar joint

- The arm must be slightly bent when taking measurements
- To ensure the best fit, don't pull the tape measure too tight, especially around flexion points (CE & CC), when making circumferential measurements.



Mobiderm MTM Armsleeve
Measurement Video

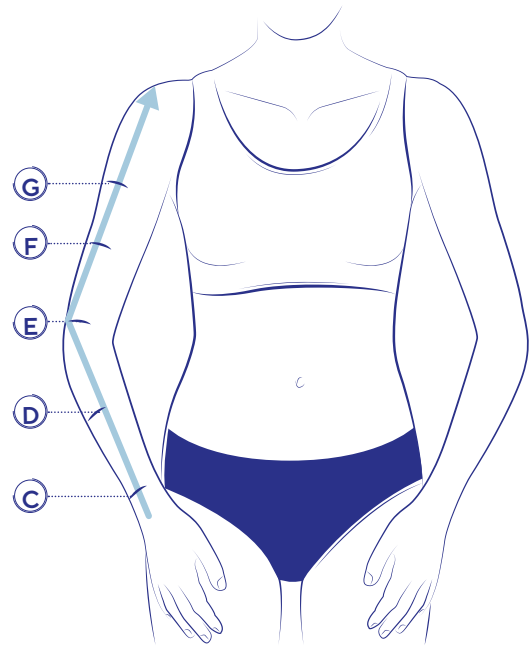


KEY: Positioning of tape measure when measuring length

Order Codes

Standard Armsleeve	3730091603
Armsleeve with Mitten, no Thumb	3730091602
Armsleeve with Mitten & Thumb	3730091601


Measurement Instructions

ARMSLEEVE

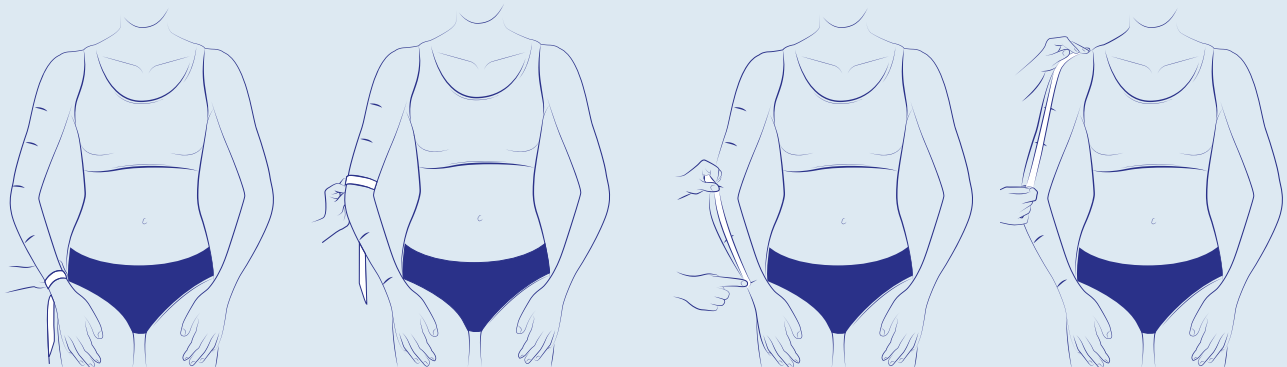

The lengths must be measured from the middle of the wrist to the tip of the elbow, then on the outside of the arm up to the desired finished height.

MITTEN

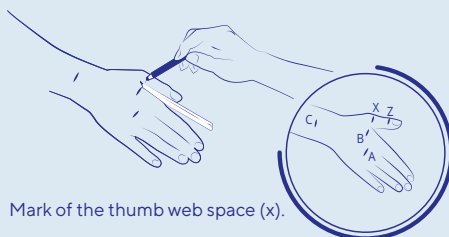

Mark of the thumb web space (x).



Measure the circumference (cx) at the base of the thumb and at the end (cz). For technical reasons, the length of the thumb (cxz) cannot be less than 2 cm.



The circumference at the end of the mitten (ca) is located at the head of the metacarpal bones.



Measure the length of the mitten:
1/ from the wrist (C) to the base of the thumb (X)
2/ from from the wrist (C) to the finished height (A)